

INSTRUCTIONS

MODEL **BHS**
SYSTEM MICROSCOPE

This instruction manual is for use of your instrument. Before putting it into operation, we recommend you read this manual carefully in order to familiarize yourself fully with its use so that you may obtain optimum performance.

OLYMPUS

AX5142

This instruction manual has been written for the use of the Olympus System Microscope Model BHS. It is recommended that you read the manual carefully in order to familiarize yourself fully with the use of the microscope, so that you can obtain optimum performance from it.

IMPORTANT

Observe the following points:

■ Operation

1. Always handle the microscope with the care it deserves, and **avoid abrupt motions**.
2. Avoid the use of the microscope in **direct sunlight, high temperature and humidity, dust and vibration**.
3. Only use the tension adjustment ring for altering the tension of the coarse adjustment knobs. (Do not twist the two coarse adjustment knobs in opposite directions simultaneously, as this will cause damage.)
4. Make it a point of grounding the microscope to prevent electric accidents.

■ Maintenance

1. Lenses must always be kept clean. Carefully wipe off oil or fingerprints deposited on the lens surfaces with gauze moistened with a **small** amount of xylene, alcohol or ether.
2. Do not use organic solutions to wipe the surfaces of various components. Plastic parts, especially, should be cleaned with neutral detergent.
3. Never disassemble the microscope for repair. Only authorized Olympus service personnel should make repairs.
4. The microscope should be covered with the vinyl dust cover provided and stored in a place free from humidity.

CONTENTS


I.	STANDARD EQUIPMENT	2
II.	NOMENCLATURE	3
III.	ASSEMBLY	4
IV.	IDENTIFICATION AND FUNCTION OF VARIOUS COMPONENTS	6
V.	OPERATION	9
	A. Switching on the Light Source	
	Voltage Adjustment and Light Intensity	
	B. Placement of a Specimen Slide	
	Cover Glass	10
	Specimen Slide	
	Stage	
	C. Observation Tube	11
	1. Interpupillary Distance Adjustment	
	2. Diopter Adjustment	
	3. Light Path Selector	
	D. Condenser Adjustment	12
	1. Condenser Centration	
	Field Iris Diaphragm	
	Aperture Iris Diaphragm	
	E. Focusing Adjustment	13
	1. Tension of Coarse Adjustment Knobs and Fine Adjustment	
	Use of Rubber Cap for Fine Adjustment Knob	
	2. Pre-Focusing Lever	
	3. Adjustment of Stage Block Height	
	F. Use of Immersion Objectives	14
	G. Photomicrography	
VI.	OPTICAL DATA	16
VII.	TROUBLESHOOTING GUIDE	17

I. STANDARD EQUIPMENT

Component		Model			
		BHS-112	BHS-113	BHS-312	BHS-313
Microscope stand	BHS-F	1	1	1	1
Observation tubes	Binocular tube BH2-BI30	1	1	0	0
	Trinocular tube BH2-TR30	0	0	1	1
Revolving nosepieces	Quintuple BH2-5RE	1	0	1	0
	Sextuple BH2-6RE	0	1	0	1
Square mechanical stage with right-hand low drive coaxial controls BH2-SVR		1	1	1	1
Condensers	Swing-out condenser BH2-SC	1	1	1	1
	Achromatic/Aplanatic condenser BH2-AAC	0	1	0	1
Halogen lamp housing BHS-LSH		1	1	1	1
Halogen bulbs 12V100WHAL-L		2	2	2	2
Objectives	D Plan 4X, D Plan 10X, D Plan 20X, D Plan 40X, D Plan 100X (oil)	1 each	0	1 each	0
	S Plan 4X, S Plan 10X, S Plan 20X, S Plan 40X, S Plan 100X (oil)	0	1 each	0	1 each
Eyepieces WHK10X		2	2	2	2
Photo eyepiece NFK3.3X		0	0	1	1
Line cord UYCP		1	1	1	1
Filter KB-4		1	1	1	1
Immersion oil, bottled		1	1	1	1
Vinyl dust cover		1	1	1	1
Allen wrench		1	1	1	1

II. NOMENCLATURE


The Model BHS consists of various components and interchangeable accessories as shown in the photo below. A wide variety of combinations, standard or optional, is available according to your requirements.

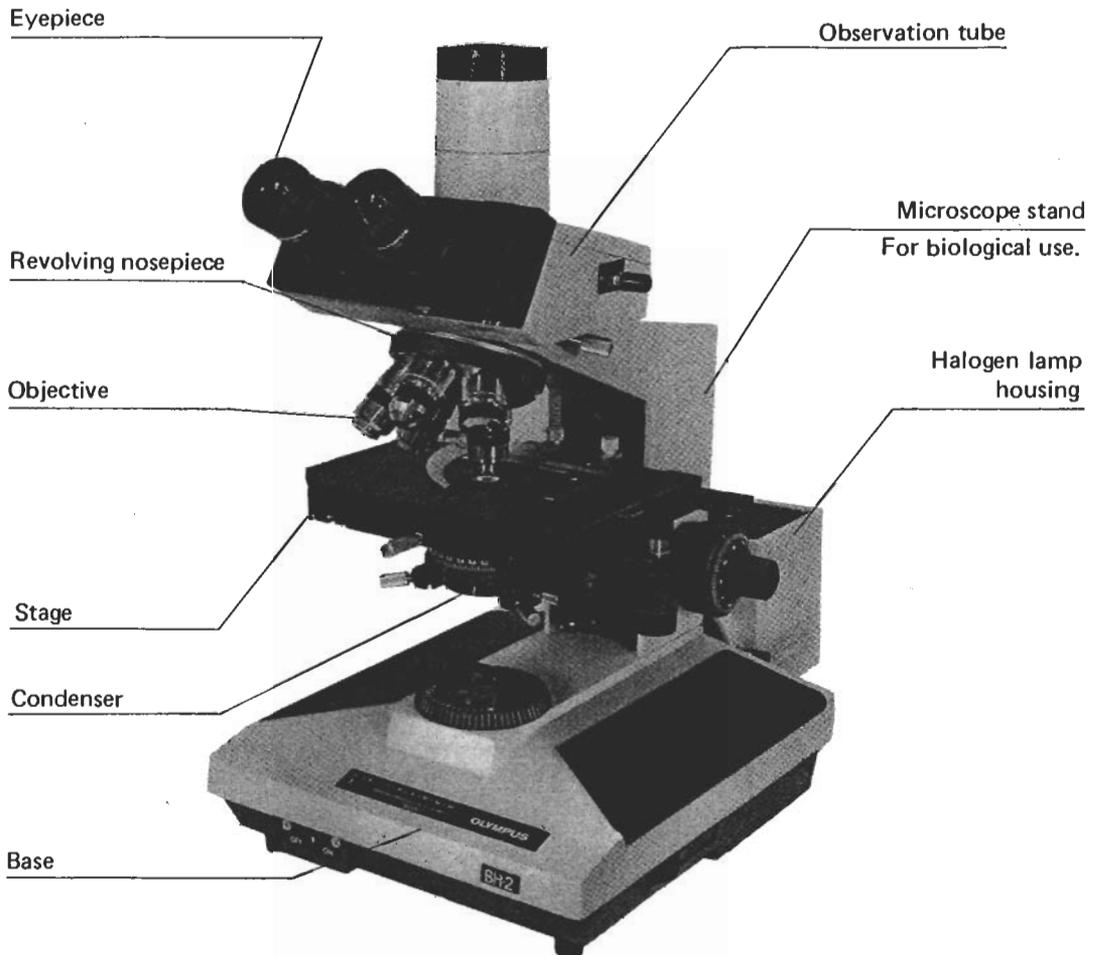

III. ASSEMBLY

This picture illustrates the sequential procedure of assembly. The numbers indicate the order of assembly of various components. Remove dust caps before mounting components. Take care to keep all glass surfaces clean, and avoid scratching the glass surfaces.

NOTE: For numbers ②, ④, ⑦ and ⑨ please refer to explanations in detail on the next page.

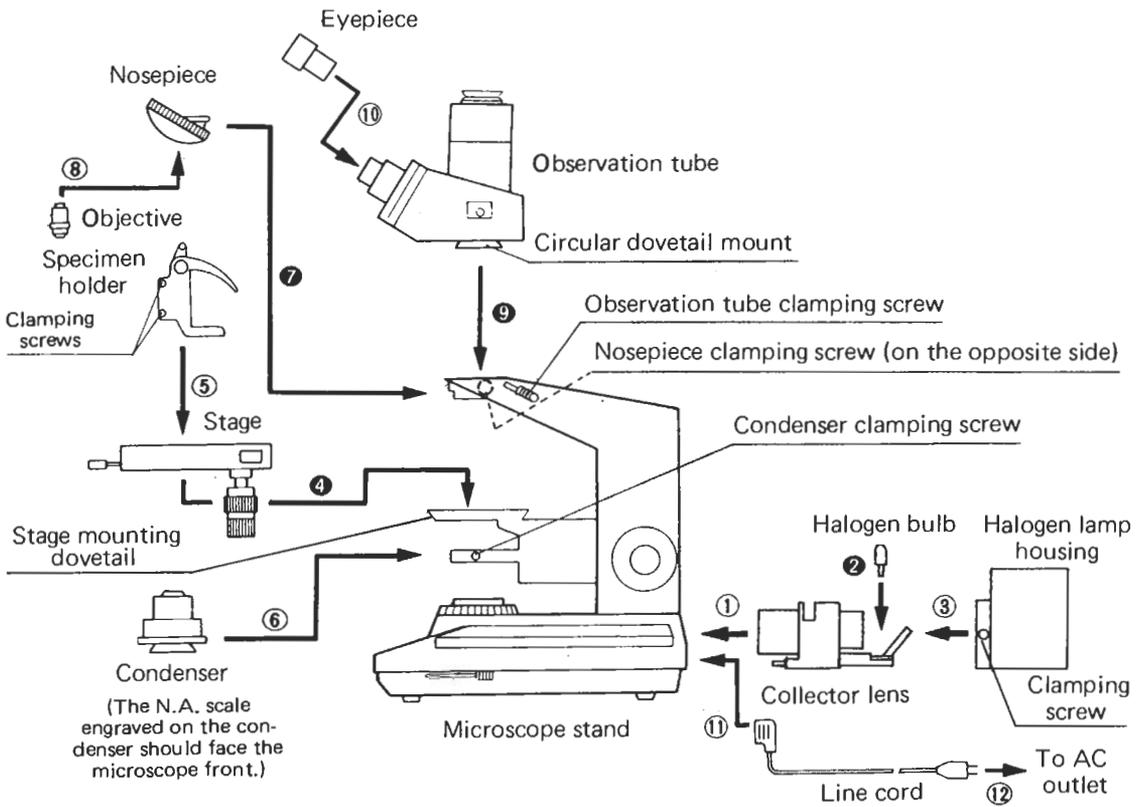

■ Explanations in detail

② Mounting the halogen bulb

- 1) Releasing the bulb clamping levers ② of the collector lens ① in the direction of the arrow, insert two contact pins of the halogen bulb into the socket ③. (Fig. 1) (Recommended to use a glove or gauze to handle the halogen bulb.)
 - 2) Secure the bulb in position with the two levers.
- ★ Before use, wipe off any fingerprints or stains on the bulb.

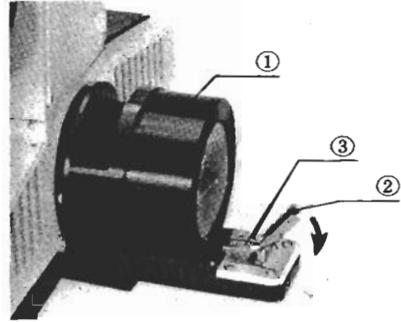


Fig. 1

④ Mounting the stage

- 1) Loosen the stage clamping screw ① by rotating counterclockwise. (Fig. 2)
- 2) Insert the stage into the mounting dovetail of the microscope stand slowly and lock with clamping screw.

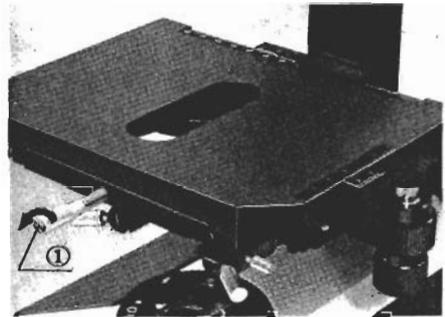


Fig. 2

⑦ Mounting the revolving nosepiece

- 1) Loosen the nosepiece clamping screw ①. (Fig. 3)
- 2) Aligning the nosepiece dovetail slide to the mounting block ②, push in the nosepiece slowly all the way.

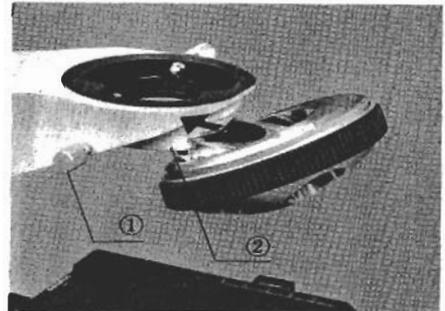


Fig. 3

⑨ Mounting the observation tube

- 1) Loosen the clamping knob ① fully. Pull spring-loaded clamping knob ①. This will cause the locating pin ② to withdraw. (Fig. 4) If the pin does not, loosen the screw further until the pin withdraws.
- 2) With clamping knob ① pulled out, insert the circular dovetail of the observation tube into the ring dovetail.
- 3) Tighten the clamping knob.



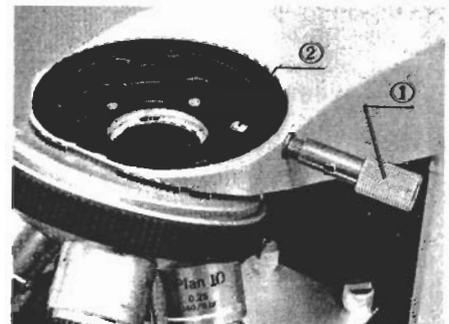


Fig. 4

IV. IDENTIFICATION AND FUNCTION OF VARIOUS COMPONENTS

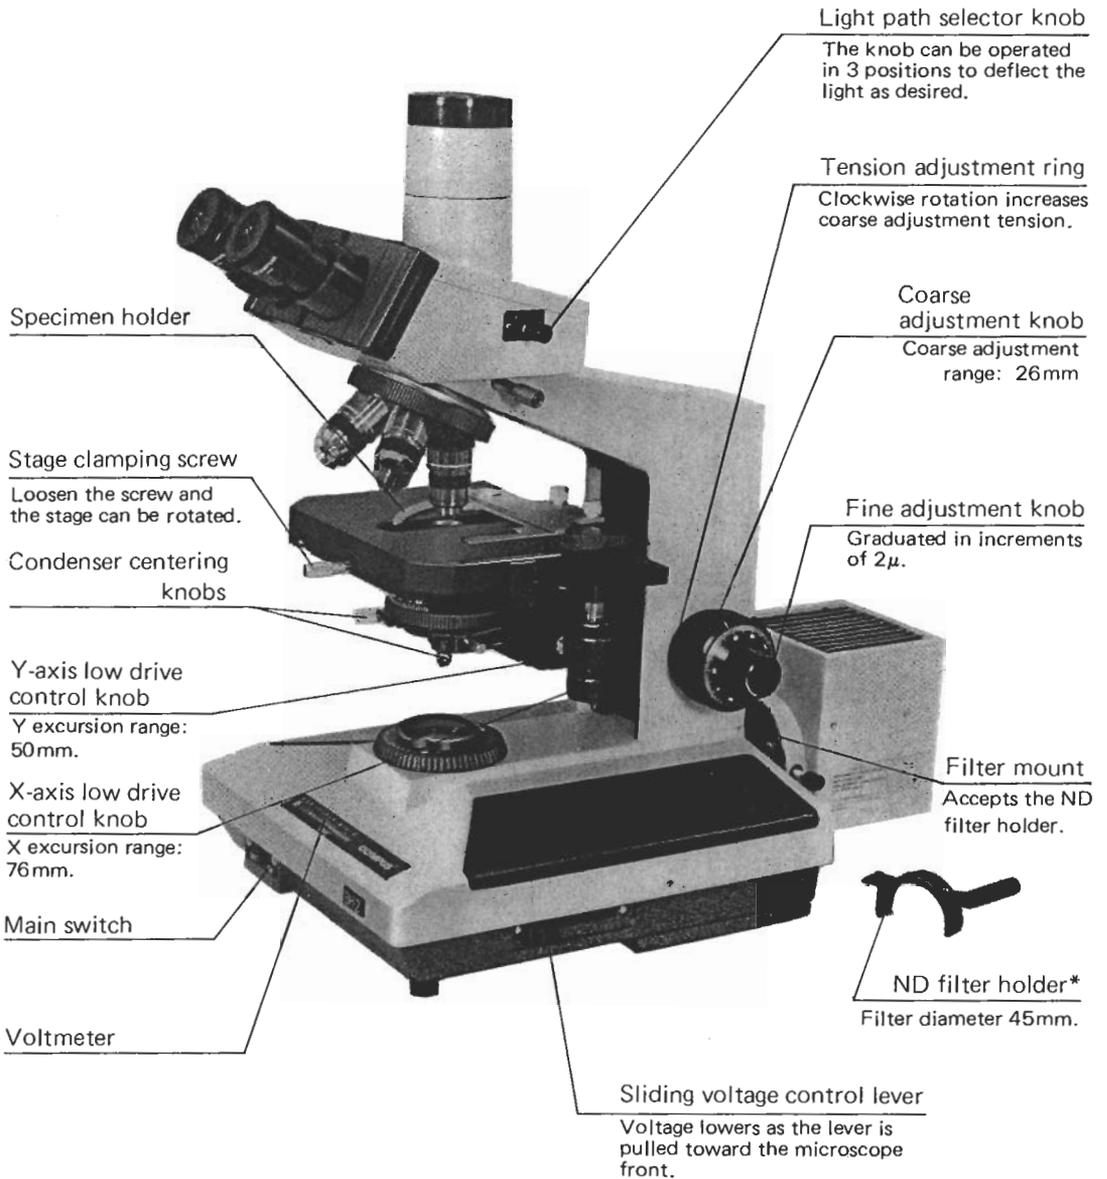

*Do not disengage the ND filter for about a few minutes after the use, in order to give time to cool. Other filters (e.g. KB-4 provided, etc.) should be inserted into the filter mount at the light exit on the microscope base.

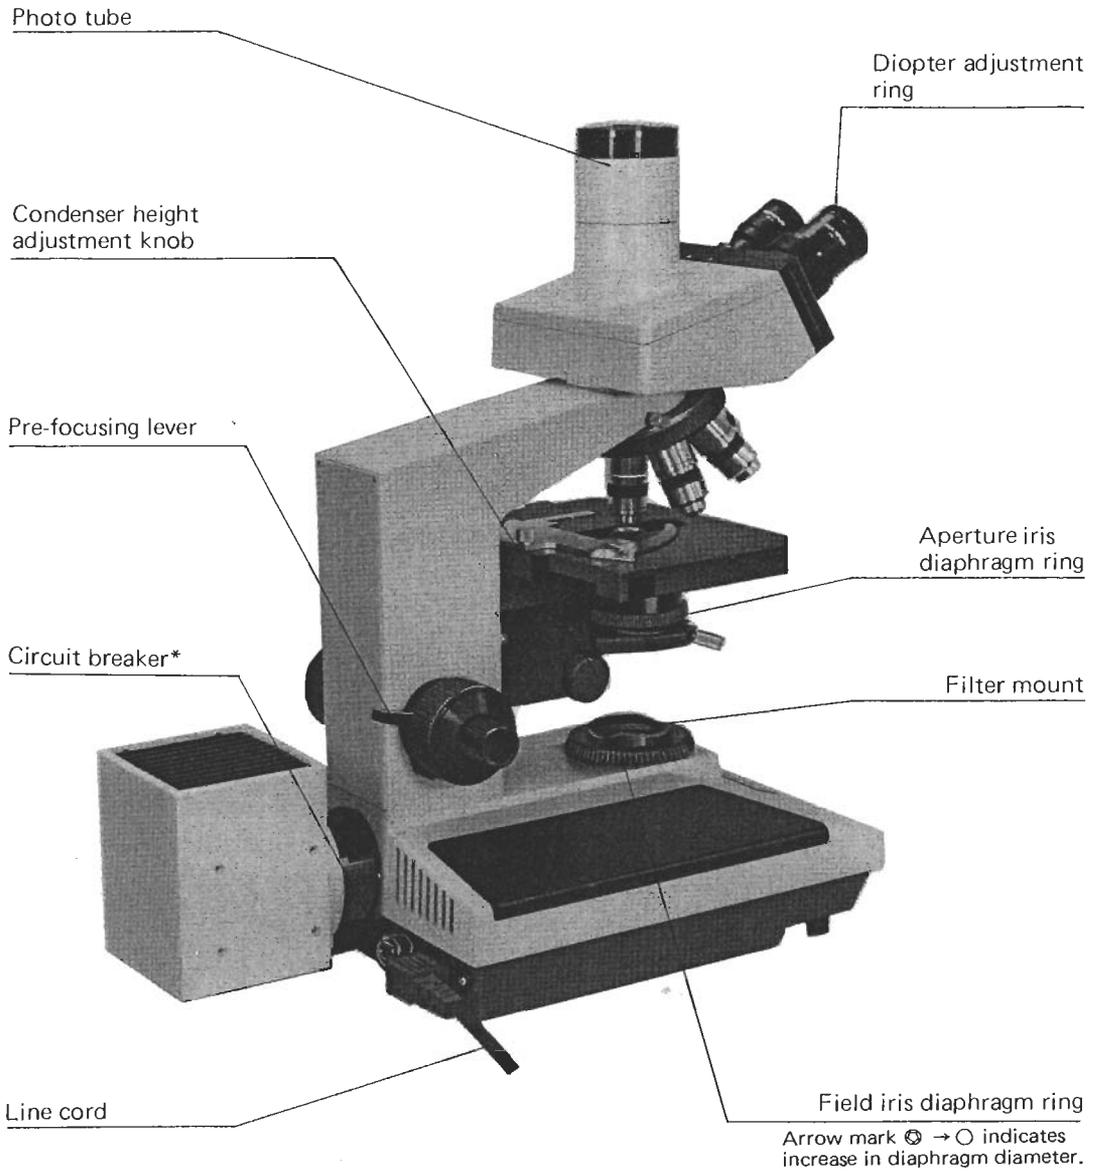

*This breaker protrudes its central part to cut off the electric power in case of the dimmer circuit trouble (due to short circuit, etc.) or over current. To restore the breaker, press the central part. If the breaker is actuated again, disconnect the line cord from the AC outlet and contact the Olympus Service Center.

Summary of Putting the Microscope into Operation

Model BHS

- A. Switch on the light source (page 9).
- B. Place a specimen slide on the mechanical stage (page 9).
- C. Coarse focus with the 10X objective.
- D. Make interpupillary distance and diopter adjustments (page 11).
- E. Adjust the condenser position (page 12).
- F. Swing in the desired objective.
- G. Adjust light intensity.
- H. Fine focus.
- I. Adjust aperture iris diaphragm and field iris diaphragm (page 12).

Adjustment of Illumination System for Various Objective Powers

Objective magnification	Condenser				
	Achromatic-aplanatic condenser BH2-AAC	Abbe condenser BH2-CD	Swing-out condenser BH2-SC	Low power condenser BH2-UL-C	
1X					
2X					Compatible
4X					
10X	Compatible	Compatible	Swing in top lens		
20X					
40X					
60X					
100X					**

*To obtain better illumination for photomicrography with a 2X objective, it is recommended to use the ultra-low condenser BH2-ULC, optionally available.

**N.A. is somewhat low, but still compatible with a 100X objective.

(Cut off this page at dotted line and put it on the wall near the microscope for use as a reminder of microscopic procedure.)

OLYMPUS

Cut Here

V. OPERATION

A. Switching on the Light Source

- 1) Place the sliding voltage control lever on the right side of the microscope base to a position closest to you (low voltage position). Switch on the light source. (Fig. 5)

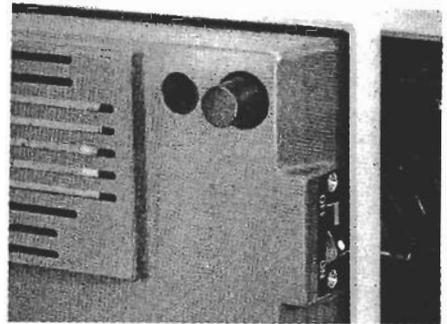


Fig. 5

Voltage Adjustment and Light Intensity

As you push the control lever ① in the direction of the arrow in order to obtain increasing intensity (Fig. 6), the LED readout ② will display the lamp voltage.

- ★ Two LEDs on the left side indicate the voltage from 0V to 6V, and twelve LEDs on the right side from 6.5V to 12V in 0.5V increments. The indication with the letters "PHOTO" can be used as a guide line for color photomicrography.

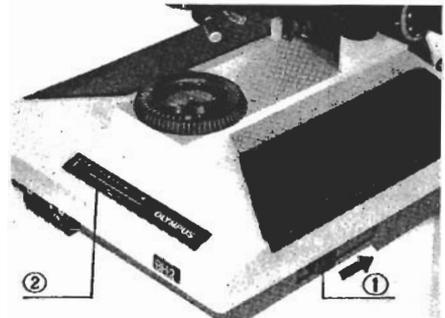


Fig. 6

B. Placement of a Specimen Slide

- 1) Rotate the coarse adjustment knobs ① in the direction of the arrow to rack down the stage so that a specimen slide can be placed on the stage. (Fig. 7)

NOTE: The rotation of the coarse and fine adjustment knobs in the direction of the arrow will rack down the stage.

- 2) Opening the spring-loaded finger of the specimen holder with one hand, place a specimen slide inside the holder. (Fig. 8) When the slide comes in contact with the back of the specimen holder, slowly return the spring-loaded finger.

WARNING: If the spring-loaded finger is returned quickly, it may cause damage to the specimen slide.

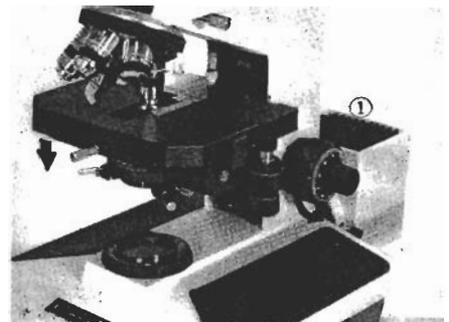


Fig. 7

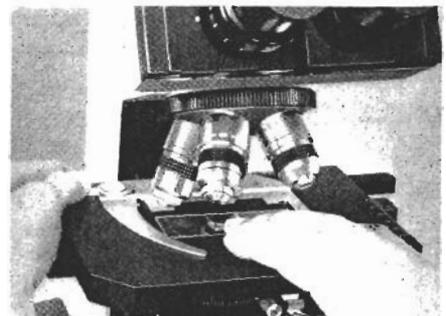


Fig. 8

Cover Glass

- An Olympus objective engraved "160/0.17" requires a cover glass of 0.17mm thickness. If the numerical aperture of the objective is 0.7 or higher (except immersion objectives) and no correction collar is provided, the resolving power deteriorates to a great extent if cover glass thickness deviates from the above listed value.

NOTE: In some countries a 0.17mm cover glass corresponds to a designation of #1½.

- A cover glass (0.4mm thick) for blood counting, etc. can be used with Olympus objectives of the working distance longer than 0.4mm. (See VI. OPTICAL DATA at page 16.)

Specimen Slide

- Specimen slides 0.8 mm to 1.2 mm thick are recommended for Olympus objectives.
- 3) Bring the portion of the specimen for observation into the light path by means of the low drive control knobs. (Fig. 9)
- ★ Tighten the stage clamping screw ① in the microscope front.

Stage

- The specimen holder can accommodate two standard specimen slides simultaneously.
- The specimen holder is removable to obtain a large unobstructed stage surface to hold specimens up to 55 mm x 85 mm.
- To rotate the stage loosen the stage clamping screw ① and holding this screw, rotate the stage into the desired direction. (Fig. 9)
- ◎ Stage clips ①, for use with immersion objectives. (Fig. 10)

A pair of stage clips are optionally available to hold the specimen on the stage, eliminating a specimen drag caused by immersion oil between slide and stage surface. The clips can be inserted into the holes provided on the specimen holder.

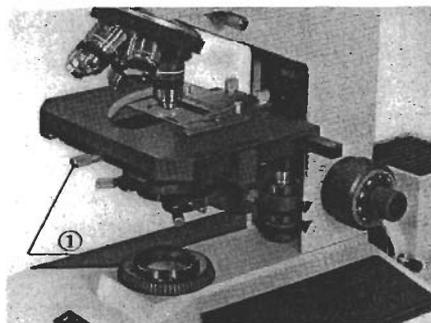


Fig. 9

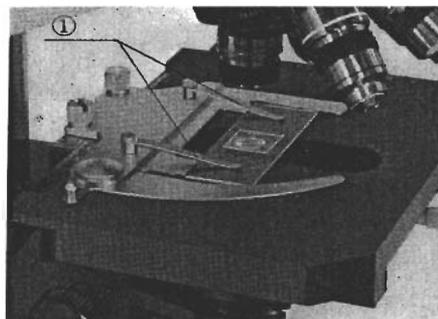


Fig. 10

C. Observation Tube

1. Interpupillary Distance Adjustment

- 1) Click the 10X objective into position.
- 2) Looking through the eyepieces with both eyes, adjust the interpupillary distance of the binocular tube by adjusting the knurled dovetail slides ① of the right and left eyepiece tubes with both hands until perfect binocular vision is obtained. (Fig. 11)

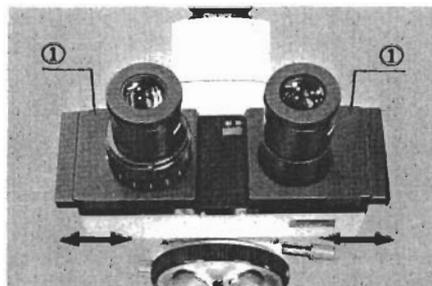


Fig. 11

2. Diopter Adjustment

- 1) Look at the image through the right eyepiece with your right eye and focus on the specimen with the fine adjustment knobs.
- 2) Next, look at the image through the left eyepiece with your left eye and rotate the diopter adjustment ring ① to focus on the specimen without using the coarse and fine adjustment knobs. (Fig. 12)

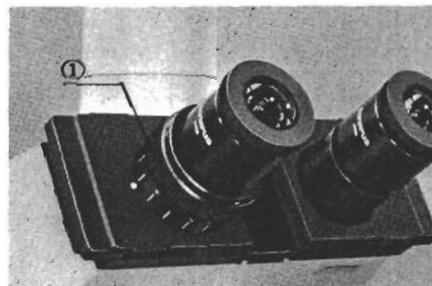


Fig. 12

3. Light Path Selection

- 1) The trinocular tube is provided with a light path selector knob ① to direct the light to the observation tube and/or to the photo tube in 3 positions (Fig. 13)

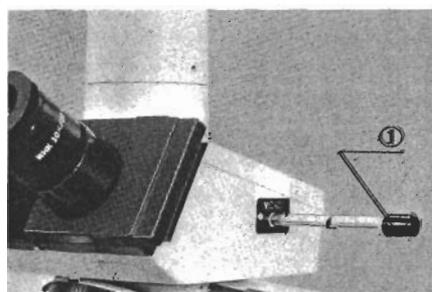


Fig. 13

Indicator Plate

	Knob Position		
	Pushed in all the way (V)	Pulled out halfway (C. V)	Pulled out all the way (C)
Amount of light	100% into binocular tube	20% into binocular tube 80% into photo tube	100% into photo tube
Application	① Observation ② Dark specimens	① Observation of excessively bright specimens ② Photomicrography (focusing through the binocular tube)	Photomicrography of dark specimens

The indicator plate is provided at the knob port to summarize the usage of the above table; it can be consulted before operating the knob.

V: Viewer (white letter)

C.V: Camera & viewer (yellow-green letters)

C: Camera (red letter)

The colors of the letters correspond with the color bands on the knob shaft.

D. Condenser Adjustment

1. Condenser Centration

- 1) Stop down the field iris diaphragm with knurled ring ① by rotating in the direction of the arrow. (Fig. 14)
- 2) Use the condenser height adjustment knob ② to move the condenser up and down until an image of the field diaphragm can be seen clearly in the eyepieces. The rotation of the knob in the direction of the arrow lowers the condenser.

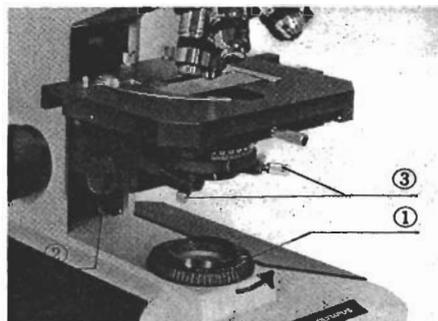


Fig. 14

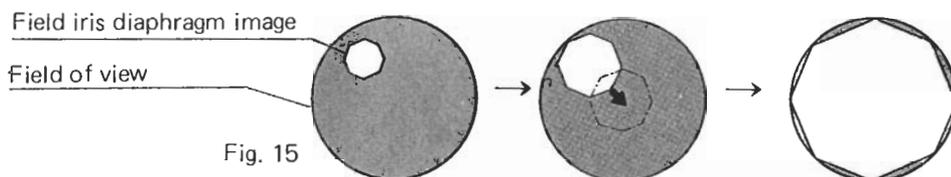


Fig. 15

- 3) Bring the field iris diaphragm image into the center of the field of view with the two condenser centering knobs ③. (Fig. 14)
- 4) Widen the diameter of the iris diaphragm progressively. If the polygonal image of the iris diaphragm becomes inscribed in the field it means that the field diaphragm is centered. (Fig. 15)

★ If the specimen slide used is thicker than 1.2 mm, you cannot obtain the image of the field iris diaphragm. Especially for photomicrography, use a specimen slide 0.9mm to 1.2 mm as much as possible.

Field Iris Diaphragm

- The field iris diaphragm controls the diameter of the ray bundle impinging on the specimen surface and therefore, by stopping down the field diaphragm until it is slightly larger than the field of view, it can reduce stray light, which in turn increases image definition and contrast.

Aperture Iris Diaphragm

- In order to achieve optimum objective performance, the opening of the aperture iris diaphragm should be matched to the numerical aperture of the objective in use. It is often preferable, however, to stop down the aperture diaphragm slightly more than indicated by the objective N.A. This will result in better image contrast, increased depth of focus and a flatter field.
- After completing focus adjustment, remove one of the eyepieces from the observation tube and look into the empty eyepiece tube. As you stop down the aperture iris diaphragm, the image of the iris diaphragm can be seen in the objective pupil. Adjust the opening of the diaphragm to match the N.A. of the objective in use. If the specimen is low in contrast, it is recommended to stop down to 70% to 80% of the objective N.A. (Fig. 16)

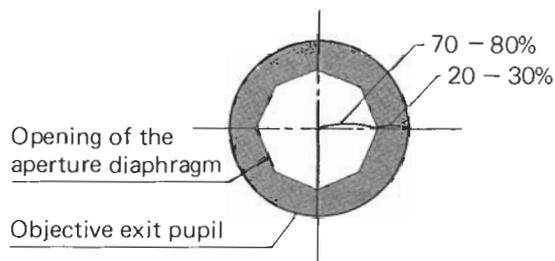


Fig. 16

E. Focus Adjustment

1. Tension of Coarse Adjustment Knobs and Fine Adjustment.

Although the tension of the coarse adjustment knobs has been already adjusted for optimum performance by the manufacturer, it is possible to personally adjust the tension of the coarse adjustment for either heavy or light movement depending on the operator's preference by rotating the tension adjustment ring ①. (Fig. 17)

The ring can be rotated by inserting a screwdriver into one of the holes on the periphery of the ring. The clockwise rotation (in the direction of the arrow) tightens the coarse adjustment knobs. Do not loosen the ring too much, because the stage may drop or the fine adjustment knobs may slip.

NOTE: Do not rotate the right and left coarse adjustment knobs in the opposite directions simultaneously. If the stage drops and the specimen goes out of focus, the tension adjustment ring is too loose. Tighten the ring.


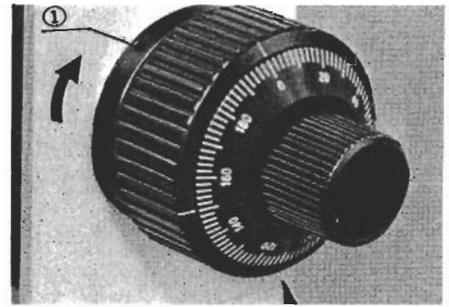


Fig. 17

Use of Rubber Cap for Fine Adjustment Knob

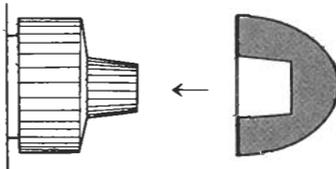

Attaching this cap over the fine adjustment knob increases the sensitivity of the fine focusing motion. (The rubber cap is optionally available.)

2. Pre-Focusing Lever

This lever ② is provided to prevent possible contact between specimen and objective as well as to simplify coarse focusing. (Fig. 18) The lever is locked after coarse focus has been accomplished. This prevents further upward travel of the stage by means of the coarse adjustment knobs, and automatically provides a limiting stop if the stage is lowered and then raised again. The pre-focusing lever does not restrict fine focusing.



Fig. 18

3. Adjustment of Stage Block Height

In addition to the vertical movement of the stage by means of coarse and fine adjustments, the stage block height can be changed for observation of specimens which are thicker than standard slides, e.g. chambers, flasks, etc. with much larger thickness.

The stage block height can be adjusted by loosening the stage block locking screw ① with the Allen wrench provided and re-tightening it at the lower position. (Fig. 19)

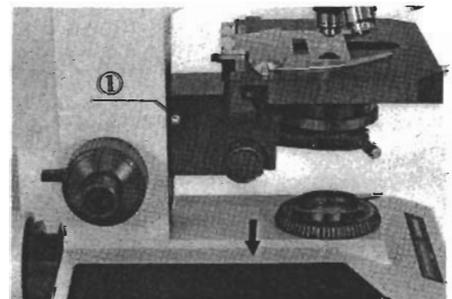


Fig. 19

F. Use of Immersion Objectives

- 1) Focus the specimen with a low power objective.
- 2) Put a drop of immersion oil on the specimen slide and the front lens of the immersion objective.
- 3) Turn the revolving nosepiece to bring the immersion objective into the light path, and focus with the fine adjustment knobs.

NOTE: ① For immersion condensers such as an achromatic-aplanatic condenser or Abbe condenser, remove the specimen from the mechanical stage and place a drop of immersion oil on the front lens of the condenser. Then, place the specimen on the stage and slowly raise the condenser until firm contact with the underside of the specimen slide is made.

② Care should be taken to prevent oil bubbles from forming in the oil film between condenser and specimen slide. If any, re-apply immersion oil, for these bubbles greatly deteriorate the lens performance.

③ After use carefully wipe off the immersion oil deposited on the lens surfaces with gauze moistened with xylene. Never leave oil on the lens surfaces after use as oil remnants will seriously impair the performance of the lens system.

G. Photomicrography

The Olympus Photomicrographic Equipment Model PM-10AD is uniquely qualified to be used with the BHS microscope for routine and advanced photomicrography. A separate, detailed instruction manual is available for the PM-10AD camera system.

For quick reference, however, you may want to refer to the following pointers when using the PM-10AD.

1. Photographic Eyepiece

Use NFK photo eyepieces for photomicrography.

Insert the eyepiece ① into the eyepiece tube of the photo tube. (Fig. 20)

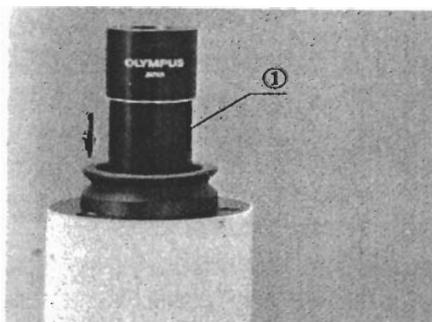


Fig. 20

2. Mounting the Photographic Unit

Slip the body of the photographic unit over the photo tube. Align the dots on photo tube and the PM-10AD body and clamp the camera unit to the photo tube. (Fig. 21)



Fig. 21

3. Setting the Light Path Selector

Refer to section C.3. on page 11.

4. Color and B & W Photomicrography

a) Color photomicrography

- Voltage setting Within a range as marked with the letters "PHOTO" on the voltmeter.
- Filter Insert the LBD-2 filter into the filter mount at the light exit on the microscope base. (in case of daylight film)
- Light intensity Should be adjusted by means of the ND filters rather than by means of voltage change.

The range of voltage setting mentioned above indicates a guide line for color photomicrography. If the photograph, taken this way, however, gives bluish tint, lower the voltage slightly, and if it gives reddish tint, raise the voltage slightly.

b) Use of contrast filters for B & W photomicrography

- ① Green filter This filter is most recommended, since it aids in obtaining photomicrographs of highest resolution and maximum contrast.
- ② Yellow filter Recommended as contrast filter when it is desirable to emphasize the blue color in the stained portion of a specimen.
- ③ Cobalt filter Not generally recommended for photomicrographic purposes since it reduces both resolution and contrast. Use it for specific applications only when it is desirable to emphasize yellow in the stained portion of a specimen.
- ④ No filter A photograph is taken with less contrast than with the green filter.

5. Focusing Procedure

Use the field of view eyepieces for focusing on the film plane. Each field of view eyepiece has a focusing front lens and a reticle with 4 frames, each frame indicating the area covered by a specific power NFK photo eyepiece. (Fig. 22).

The number at each frame indicates the magnification of the photo eyepiece. The image in the field of view eyepiece and the image on the film plane are in focus at the same time. Several type field of view eyepieces are available, according to the film size employed.




Fig. 22

Field of view eyepiece	35WHK10X	PWHK10X	4X5WHK10X	MHWHK10X
Attachment camera	35mm Back	3¼" x 4¼" Polaroid Back	4" x 5" Sheet Film or Polaroid Film Holder	16 mm Bolex camera 120 Roll Film Holder

- 1) Select the field of view eyepiece matching the camera back in use and insert it into the right eyepiece tube of the trinocular tube, aligning locating groove and locating pin.
- 2) While looking through the field of view eyepiece, rotate the eyepiece front lens in screw mount to focus on the double cross lines in the field. For sharp focusing with objectives 4X or lower, the focusing magnifier FT is recommended.
- 3) Bring the specimen detail to be photographed within the frame corresponding to the power of the NFK eyepiece in use and focus on the specimen with the microscope fine adjustment knobs. Make sure the light path selector knob on the observation tube is either on the white (V) or yellow-green (CV) band.
- 4) It is recommended to tighten the tension adjustment ring considerably to prevent the stage from dropping during long exposures.

VI. OPTICAL DATA

Objective	Type	D Plan Ach.					S Plan Ach.				
	Eyepiece	Magnification	4X	10X	20X	40X	100X*	4X	10X	20X	40X
N.A.		0.10	0.25	0.40	0.65	1.25	0.13	0.30	0.46	0.70	1.25
W.D. (mm)		7.03	7.4	0.83	0.23	0.17	15.5	7.5	1.5	0.5	0.17
Focal length (mm)		34.23	17.69	8.99	4.61	1.75	36.54	18.98	8.03	4.13	1.69
Resolving power (μ)		3.36	1.34	0.84	0.52	0.27	2.58	1.12	0.73	0.48	0.27
WHK 10X (Field number 20)	Total mag.	40X	100X	200X	400X	1000X	40X	100X	200X	400X	1000X
	Focal depth (μ)	173	27.6	9.15	3.0	0.68	125.4	22.1	7.6	2.72	0.68
	Field of view (mm)	5	2	1	0.5	0.2	5	2	1	0.5	0.2

*Immersion objectives

The resolving power and focal depth are obtained with fully opened aperture diaphragm.

Technical terms:

- Working distance: The distance from the cover glass to the nearest point of the objective.
- Numerical aperture: The N.A. represents a performance number which can be compared to the relative aperture (f-number) of a camera lens. The N.A. values can be used for directly comparing the resolving powers of all types of objectives. The larger the N.A., the higher resolving power.
- Resolving power: The ability of a lens to register small details. The resolving power of a lens is measured by its ability to separate two points.
- Focal depth: The distance between the upper and lower limits of sharpness in the image formed by an optical system. As you stop down the aperture iris diaphragm, the focal depth becomes larger. The larger the N.A. of an objective the shallower the focal depth.
- Field number: A number that represents the diameter in mm of the image of the field diaphragm that is formed by the lens in front of it.
- Field of view diameter: The actual size of the field of view in mm on the object surface.

VII. TROUBLESHOOTING GUIDE

If you are unable to obtain full performance from your microscope, please consult with the table below as pointers for troubleshooting.

Phenomenon	Cause	Remedy
1. Optical System		
a) With illuminator switched on, the field of view is dark.	Field iris diaphragm is not opened sufficiently.	Open diaphragm to proper diameter.
	Condenser is lowered too much.	Adjust condenser height.
	Light path selector lever is pulled out to C position.	Push in lever up to CV or V position.
b) Field of view is cut off or illuminated irregularly.	Light path selector lever is stopped midway.	Click it into proper position according to your purpose.
	Nosepiece is not clicked into place.	Slightly rotate nosepiece until it clicks into place.
	Nosepiece is not correctly mounted.	Insert nosepiece dovetail into microscope frame all the way, then lock.
	The power of objective used exceeds the illumination capacity of condenser.	Choose a condenser to meet your purpose.
	Condenser is not centered.	Center condenser.
	Field iris diaphragm is stopped down excessively.	Open diaphragm to proper diameter.
c) Dust or dirt is visible in the field of view.	Dust, etc. on light exit lens.	Remove dust, etc. Clean front lenses.
	Dust on condenser top lens.	
	Dirty specimen.	
	Dust on eyepiece.	
d) Excessive image contrast.	Condenser is lowered too much.	Adjust condenser height.
	Aperture iris diaphragm is stopped down excessively.	Open diaphragm to proper diameter.

Phenomenon	Cause	Remedy
e) Resolution problems: <ul style="list-style-type: none"> • Image is not sharp. • Insufficient contrast. • Image details lack definition. 	Non Olympus objectives are used.	Use Olympus LB series objectives.
	Nosepiece is not correctly mounted.	Insert nosepiece dovetail into microscope frame all the way, then lock.
	Objective is not correctly positioned in the light path.	Click nosepiece into place.
	Objective correction collar is not adjusted.	Rotate correction collar, keeping specimen in fine focus until optimum resolution is obtained.
	Dust on objective front lens.	Clean front lens.
	Immersion objective is not used with immersion oil.	Use immersion oil.
	Bubbles in immersion oil.	Remove bubbles (and reapply oil).
	Immersion oil designated by Olympus is not used.	Use Olympus immersion oil.
	Dirty specimens.	Clean.
	Dust on condenser lens.	
f) Field of view is partially out of focus, or image is partly out of focus.	Nosepiece is not correctly mounted.	Insert nosepiece dovetail into microscope frame all the way, then lock.
	Objective is not correctly positioned in the light path.	Slightly rotate nosepiece until it clicks in place.
	Specimen is not correctly positioned on stage.	Place specimen slide correctly on stage, and place stage clips open it.
g) Specimen image is partially out of focus.	Nosepiece is not correctly mounted.	Insert nosepiece dovetail into microscope frame all the way, then lock.
	Objective is not correctly positioned in the light path.	Slightly rotate nosepiece until it clicks into place.
	Condenser is not centered.	Center condenser.
h) Field of view becomes only slightly brighter by increasing voltage.	Condenser is not correctly centered.	Center condenser.
	Condenser is lowered too much.	Adjust condenser height.

Phenomenon	Cause	Remedy
2. Electric System		
a) Lamp goes off and on.	Bulb filament is likely to burn out.	Replace bulb.
	Loose electric connections.	Check all connections.
b) Bulb burns out frequently.	Bulb is not standard one.	Use standard bulb.
3. Coarse and Fine Adjustments		
a) Coarse adjustment knob is too tight.	Tension adjustment ring is tightened too much.	Loosen ring properly.
	User is trying to raise stage above the focusing limit imposed by the engaged pre-focusing lever.	Unlock lever.
b) Stage drops or specimen goes out of focus during observation due to slipping fine adjustment knobs.	Tension adjustment ring is too loose.	Tighten ring properly.
c) Stage cannot be raised to the upper limit.	Pre-focusing lever is engaged in lower than focusing position.	Unlock lever.
d) Stage cannot be lowered to the lower limit.	Stage is mounted too low.	Raise stage mount with Allen wrench.
e) Objective front lens hits specimen before coming into focus.	Specimen is placed on stage upside down.	Reverse specimen.
4. Observation Tubes		
a) Incomplete binocular vision.	Interpupillary distance is not correctly adjusted.	Correct the interpupillary distance.
	Diopter adjustment is incomplete.	Complete the diopter adjustment.
	Right and left eyepieces are not matched.	Use a pair of matched eyepieces.
	User is unaccustomed to binocular vision.	Prior to looking into the binocular observation tube, look at a far away object.
5. Stage		
a) Image easily goes out of focus when you touch the stage.	Stage is not correctly locked.	Clamp stage securely.
b) Specimen stops midway on the east-west traverse.	Specimen is not correctly positioned.	Adjust specimen position .

OLYMPUS

OLYMPUS OPTICAL CO., LTD.

San-Ei Building, 22-2, Nishi Shinjuku 1-chome, Shinjuku-ku, Tokyo, Japan

OLYMPUS OPTICAL CO., (EUROPA) GMBH.

Postfach 104908, Wendenstrasse 14-16, 2000 Hamburg 1, West Germany

OLYMPUS CORPORATION

4 Nevada Drive, Lake Success, N.Y. 11042-1179, U.S.A.

OLYMPUS OPTICAL CO. (U.K.) LTD.

2-8 Honduras Street, London EC1Y0TX



The design of the product is under constant review and whilst every effort is made to keep this manual up to date, the right is reserved to change specifications and equipment at any time without prior notice.